



AEGIS PEPTIDE ANALYTICS

Certificate of Analysis

Independent Third-Party Testing Laboratory



CERTIFICATE NO.

APA-2026-000069

✓ OVERALL PASS

SAMPLE INFORMATION

COMPOUND: Cerebrolysin
CAS NUMBER: 12656-61-0
ISSUE DATE: August 16, 2026

LOT NUMBER: NOVA7X
TEST DATE: August 15, 2026
TESTING METHODS: HPLC-UV · LC-MS/MS · ICP-MS ·
LAL · Karl Fischer

TEST RESULTS

01 Purity Analysis: HPLC-UV

USP <621>, Reverse-Phase C18, UV 220 nm

PURITY RESULT

99.2%


SPECIFICATION

≥ 99.0%

RESULT

✓ PASS

CHROMATOGRAM (ILLUSTRATIVE, REVERSE PHASE C18, 220 NM)

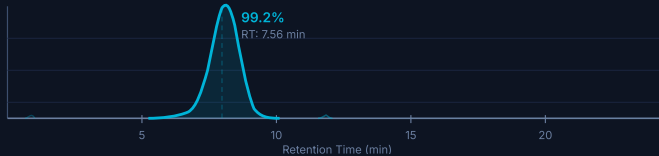

DETECTION λ
220 nm

RETENTION TIME
7.56 min

PEAK AREA
N/A

COLUMN
C18 150×4.6mm 5μm

02 Identity Confirmation: LC-MS/MS

ESI positive mode, Triple Quadrupole, USP <621>

MOLECULAR FORMULA

Multi-peptide Composition

✓ CONFIRMED

EXPECTED MW
N/A

OBSERVED [M+H]⁺
Characteristic peptide
fingerprint confirmed

MASS ERROR
N/A

Cerebrolysin is a standardized mixture of neuropeptides. Identity confirmed via characteristic LC-MS/MS peptide fingerprint analysis.

03Heavy Metals Screening: ICP-MS

ICP-MS, USP <232>/<233>

ELEMENT	SYMBOL	RESULT (PPB)	LIMIT (PPB)	STATUS
Lead	Pb	<0.5	500	✓ PASS
Arsenic	As	<0.3	1,500	✓ PASS
Mercury	Hg	<0.1	300	✓ PASS
Cadmium	Cd	<0.2	500	✓ PASS
Chromium	Cr	<1.0	1,100	✓ PASS
Nickel	Ni	<1.0	2,000	✓ PASS
Copper	Cu	<2.0	3,000	✓ PASS
Cobalt	Co	<0.5	500	✓ PASS

04Bacterial Endotoxins: LAL

Kinetic Turbidimetric LAL, USP <85>

ENDOTOXIN RESULT	ACCEPTANCE LIMIT	LAL SENSITIVITY	RESULT
<0.25 EU/mL	1 EU/mL	0.125 EU/mL	✓ PASS

05Water Content: Karl Fischer Titration

Volumetric Karl Fischer Titration, USP <731>

WATER CONTENT	SPECIFICATION	RESULT
5.5%	≤ 8.0%	✓ PASS

Content vs. Limit (5.5% / 8.0%)

METHODOLOGY & QUALITY REFERENCES

All analytical procedures are performed in compliance with the current United States Pharmacopeia (USP), International Council for Harmonisation (ICH) guidelines, and applicable FDA Analytical Procedures guidance documents. Reference standards are NIST-traceable or USP-grade. Instruments are calibrated per manufacturer protocols and internal SOPs with documented calibration records. All results are issued as final and cannot be retroactively altered after certificate issuance.

- USP <61>/<62>
- USP <71>
- USP <85>
- USP <232>/<233>
- USP <621>
- USP <731>
- USP <788>
- ICH Q3C
- ICH Q2(R2)

CHAIN OF CUSTODY			
Sample Received	Analysis Start	Analysis Complete	Certificate Issued
N/A	August 15, 2026	August 15, 2026	August 16, 2026

Authorized Laboratory Signatory
Lab Director / Quality Manager

Date of Release
August 16, 2026

